



1. Remove the protective cover from the bottom of the card.

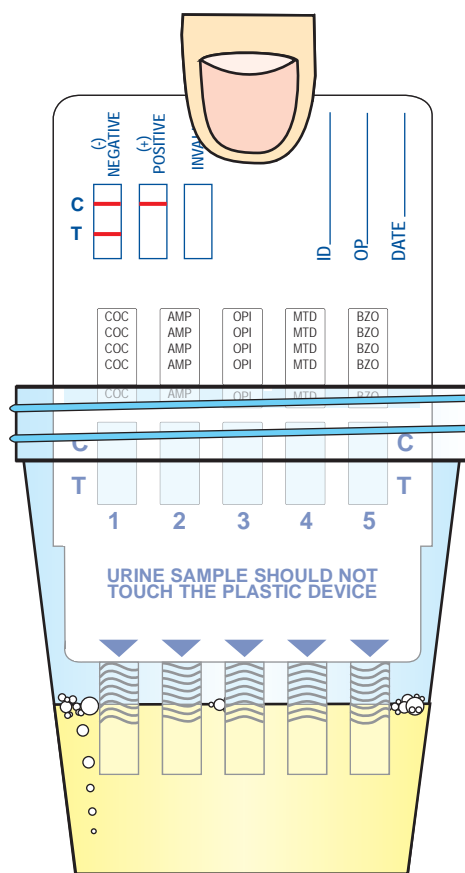

2. Immerse the card into the urine sample for 10 seconds. Urine sample should not touch the plastic device.

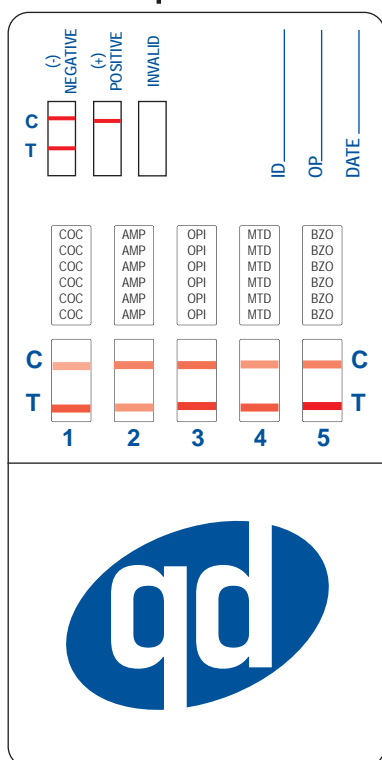

3. Replace the protective cover, read the results of the test after 5 minutes and record the results. (Here 5 negative results shown).



Note: Line colour & intensity may vary as seen here.